

Quality Assessment Report for Water Quality Monitoring

January – March 2015



**Submitted to the
Technical Oversight Committee
July 10, 2015**

Zdzislaw Kolasinski (zkolasin@sfwmd.gov)

**Analytical Services
Water Quality Bureau
South Florida Water Management District
West Palm Beach, Florida**

INTRODUCTION

This report is an assessment of the South Florida Water Management District (SFWMD) laboratory analysis and field sampling for total phosphorus (TP) monitoring, primarily for the following projects and their associated stations from January 1, 2015, through March 31, 2015.

- Everglades National Park Inflows North (PIN): S12A, S12B, S12C, S12D, S333, S355A, S355B, and S356-334
- Everglades National Park Inflow East (PIE): S332DX, S18C, DS4, and BERMB3
- Everglades Protection Area (EVPA): LOX3 through LOX16

Because field quality control (QC) samples are collected for sampling events that include multiple project samples for the stations of interest, the report may also cover information on stations or projects other than those in the above list.

The SFWMD's *Field Sampling Quality Manual* (SFWMD 2015b) provides the minimum requirements followed in field sample collection. The *Chemistry Laboratory Quality Manual* (SFWMD 2015a) provides the minimum requirements followed in preparing and analyzing laboratory samples, as well as data verification and validation. The Field Sampling Quality Assessment and Laboratory Analysis Quality Assessment sections in this report provide the field and laboratory QC results during this quarter. The SFWMD's Laboratory Information Management System (LIMS) provided the data used in this report. These data are available in the SFWMD's DBHYDRO database. Appendix A contains all TP results for samples of interest to the Everglades Technical Oversight Committee (TOC), collected from January 1, 2015 through March 31, 2015.

This report includes an analysis of the SFWMD laboratory's performance on the EVPA split samples with the Florida Department of Environmental Protection (FDEP) for a one-year period. The report also includes the results of the National Water Research Institute Environment Canada Ecosystem Inter-laboratory Proficiency Testing Program.

FIELD SAMPLING QUALITY ASSESSMENT

PROCEDURE UPDATES

This period had no major procedural updates related to TP sample collection.

SAMPLES NOT COLLECTED

Table 1 lists the 41 samples that were not collected for this reporting period. Samples were not collected due to lack of flow, dry site, shallow water depth, insufficient water level, or site under construction.

Table 1. List of samples not collected from January 1, 2015 to March 31, 2015.

Project	Collection Date	Station	Comments
PIN	01/05/2015	S12B	No flow, no sample collected
PIN	01/05/2015	S12C	No flow, no sample collected
PIN	01/05/2015	S12C	No flow, no sample collected
PIE	01/06/2015	BERMB3	Site dry
PIN	01/12/2015	S12B	No flow, no sample collected
PIN	01/12/2015	S12C	No flow, no sample collected
PIN	01/20/2015	S12B	No flow, no sample collected
PIN	01/20/2015	S12C	No flow, no sample collected
PIN	01/26/2015	S12B	No flow, no sample collected
PIN	01/26/2015	S12C	No flow, no sample collected
PIN	01/26/2015	S333	Gate removed for repair, no sample collected
PIN	02/02/2015	S12B	No flow, no sample collected
PIN	02/02/2015	S12C	No flow, no sample collected
PIN	02/02/2015	S333	Site under construction, no sample collected
PIE	02/03/2015	BERMB3	Site dry
PIN	02/09/2015	S12B	No flow, no sample collected
PIN	02/09/2015	S12C	No flow, no sample collected
PIN	02/09/2015	S333	Site under construction, no sample collected
PIN	02/16/2015	S12B	No flow, no sample collected
PIN	02/16/2015	S12C	No flow, no sample collected
PIE	02/17/2015	BERMB3	Site dry
PIN	02/23/2015	S12B	No flow, no sample collected
PIN	02/23/2015	S12C	No flow, no sample collected
PIN	02/23/2015	S333	Site under construction, no sample collected
PIN	03/02/2015	S12B	No flow, no sample collected
PIN	03/02/2015	S12C	No flow, no sample collected
PIN	03/02/2015	S333	Site under construction, no sample collected
PIE	03/03/2015	BERMB3	No flow, no sample collected
PIN	03/09/2015	S12B	No flow, no sample collected
PIN	03/09/2015	S12C	No flow, no sample collected
PIN	03/16/2015	S12B	No flow, no sample collected
PIN	03/16/2015	S12C	No flow, no sample collected
PIN	03/16/2015	S12D	No flow, no sample collected
PIE	03/17/2015	BERMB3	No flow, no sample collected
PIN	03/23/2015	S12B	No flow, no sample collected
PIN	03/23/2015	S12C	No flow, no sample collected
PIN	03/23/2015	S12B	No flow, no sample collected
PIN	03/30/2015	S12B	No flow, no sample collected
PIN	03/30/2015	S12C	No flow, no sample collected
PIN	03/30/2015	S12B	No flow, no sample collected

FIELD QUALITY CONTROL

Field QC measures consist of field generated equipment blanks (EB), field-cleaned equipment blanks (FCEB), field blanks (FB), split samples (SS), and replicate samples (RS). **Table 2** summarizes EB, FCEB, and FB results for projects of interest to the TOC, as referenced in the table's footnotes. **Table 3** summarizes the field precision results and shows that the field sampling precision was acceptable for all three project replicates.

Table 2. Field and equipment TP blank results.

Type of Blank	Project	Number of Blanks Collected	Number of Blanks With Analyte Detected
EB	EVPA	1	0
	PIE	1	0
	PIN	2	0
FCEB	EVPA	6	0
	PIE	24	0
	PIN	12	0
FB	EVPA	0	0
	PIE	7	0
	PIN	15	0
Total		68	0

Notes:

- All blanks were from sampling events containing grab and auto-sampler samples collected during the sampling event on the day of collection or day adjacent to the collection date for the compliance samples.
- FCEB, EB, and FB acceptance criteria: they must be less than the method detection limit (MDL).
- When sample concentrations are less than 10 times the blank values that were equal or greater than the MDL, the qualifier "G" is assigned to the associated sample(s).
- MDL – 0.002 mg/L

Table 3. Precision summary for TP field replicates.

Project Code	Number of Samples (Replicates)	Date Collected	Station	% RSD	Average Value (mg/L)	Comments
PIE	3	01/05/2015	S331-173*	10.8	0.005	The precision criterion was met.
PIN	3	01/06/2015	US41-25*	3.1	0.018	The precision criterion was met.
EVPA	3	02/17/2015	CA316*	10.2	0.006	The precision criterion was met.
EVPA	3	03/04/2015	LOX16	15.7	0.007	The precision criterion was met.

Notes:

- The SFWMD's chemistry laboratory conducted all TP analyses.
- Field precision must be ≤ 20 percent. The laboratory applied this criterion only if sample values were greater than the practical quantitation limit (PQL).
- % RSD – percent relative standard deviation.
- mg/L – milligrams per liter.
- *The replicate samples were collected at the stations different than stations of interest, which are listed in the Introduction section.
- I - indicates the reported value is greater than or equal to the MDL but less than the PQL.

FIELD AUDIT

The SFWMD did not conduct any field audits on TOC-related projects during the first quarter of 2015.

LABORATORY ANALYSIS QUALITY ASSESSMENT

PROCEDURE UPDATES

The TP analytical procedure (Standard Methods 4500 P-F, Automated Ascorbic Acid Reduction Method) did not change during this reporting period.

LABORATORY QUALITY CONTROL

Routine laboratory QC samples include QC checks, matrix spikes, and precision checks. **Figures 1 through 7** show the TP recoveries from various types and levels of QC samples at the SFWMD laboratory from January 1, 2015 through March 31, 2015. Control charts provide a graphical means to demonstrate statistical control, monitor a measurement process, diagnose measurement problems, and document measurement uncertainty. They also are used to monitor and document critical aspects of samples and sampling operation.

Figure 1 shows the recoveries for a laboratory control sample (LCS1) at a TP concentration of 0.300 milligrams per liter (mg/L). Performance limits varied from 97 to 102 percent, and had a mean central line value of 99.7 percent based on 471 results. The acceptable control limit is 90–110 percent.

Figure 2 shows the recoveries for a laboratory control sample (LCS3) at a TP concentration of 0.020 mg/L. Performance limits varied from 90 to 107 percent, and had a mean central line value of 98.4 percent based on 80 results. The acceptable control limit is 90–110 percent.

Figure 3 shows the recoveries for a continuing calibration verification sample (CCV) at a TP concentration of 0.200 mg/L. Performance limits varied from 98 to 102 percent, and had a mean

central line value of 99.8 percent based on 391 results. The acceptable control limit is 90–110 percent.

Figure 4 shows the recoveries for the method detection limit (MDL) sample (LCS5) at a TP concentration 0.004 mg/L and results varied from 0.003 to 0.005 mg/L based on 80 results.

Figure 5 show the recoveries for the practical quantitation limit (PQL) varied from 75 to 125 percent. The acceptable control limit is 55–145 percent.

Figures 6 and 7 present the precision and matrix spike recoveries for TP analyses during the reporting period. If QC recoveries are outside the set limits, then the SFWMD’s laboratory usually rejects the analytical batch and re-analyzes.

The acceptable recoveries for the QC samples, except the PQL check, are within ± 10 percent of the true value. The daily MDL check with a true value of 0.004 mg/L indicates that the laboratory has consistently achieved the established MDL of 0.002 mg/L. The mean recovery for the organic check, a solution prepared from phytic acid and used to prepare matrix spikes, was 98.2 percent based on 303 results.

Figures 1 through 7 show also the distribution of QC samples (histograms) in the roughly symmetrical bell-shape form with most values clustered around the central line.

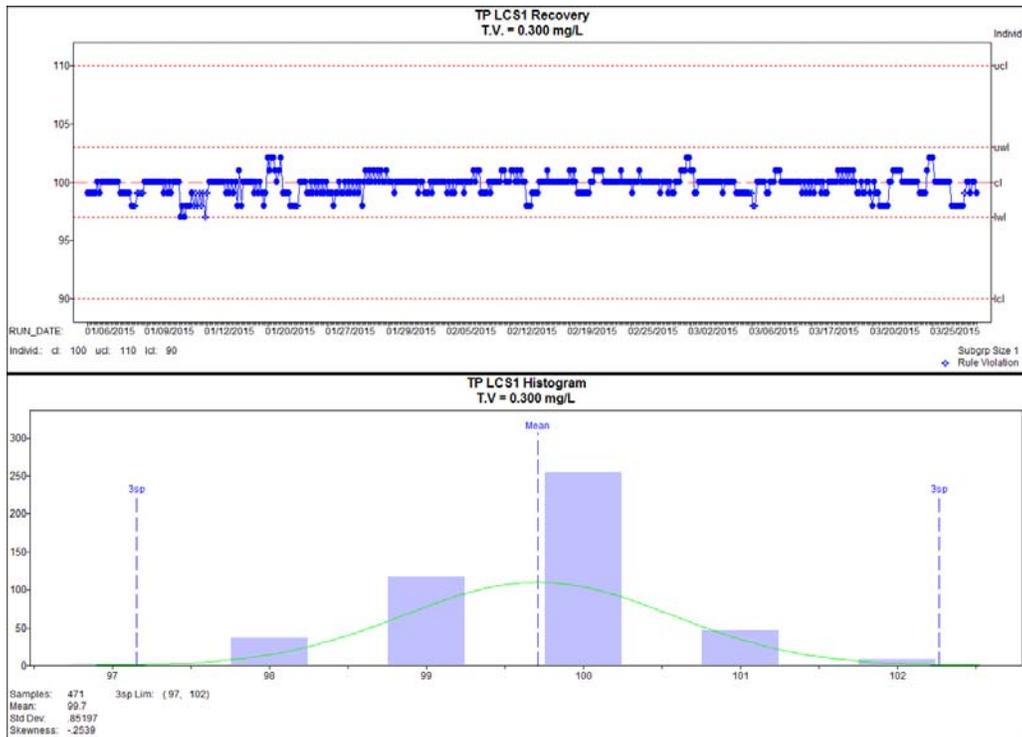


Figure 1. TP QC (Laboratory Control Sample 1, 0.300 mg/L) sample recoveries and histogram.

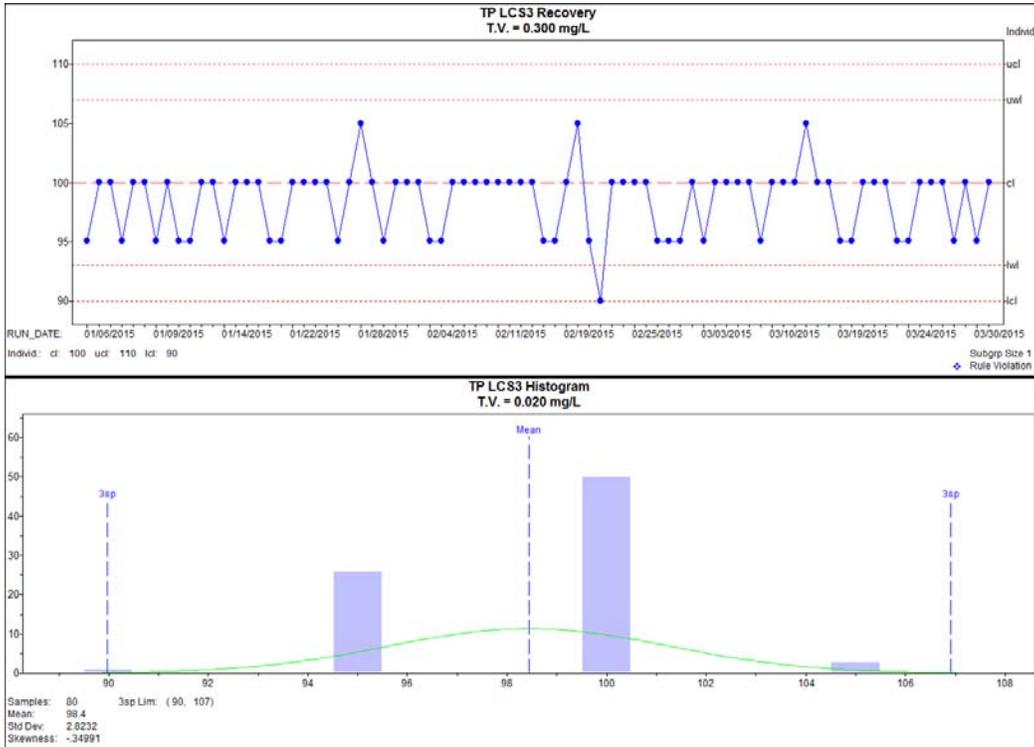


Figure 2. TP QC (Laboratory Control Sample 3, 0.020 mg/L) sample recoveries and histogram.

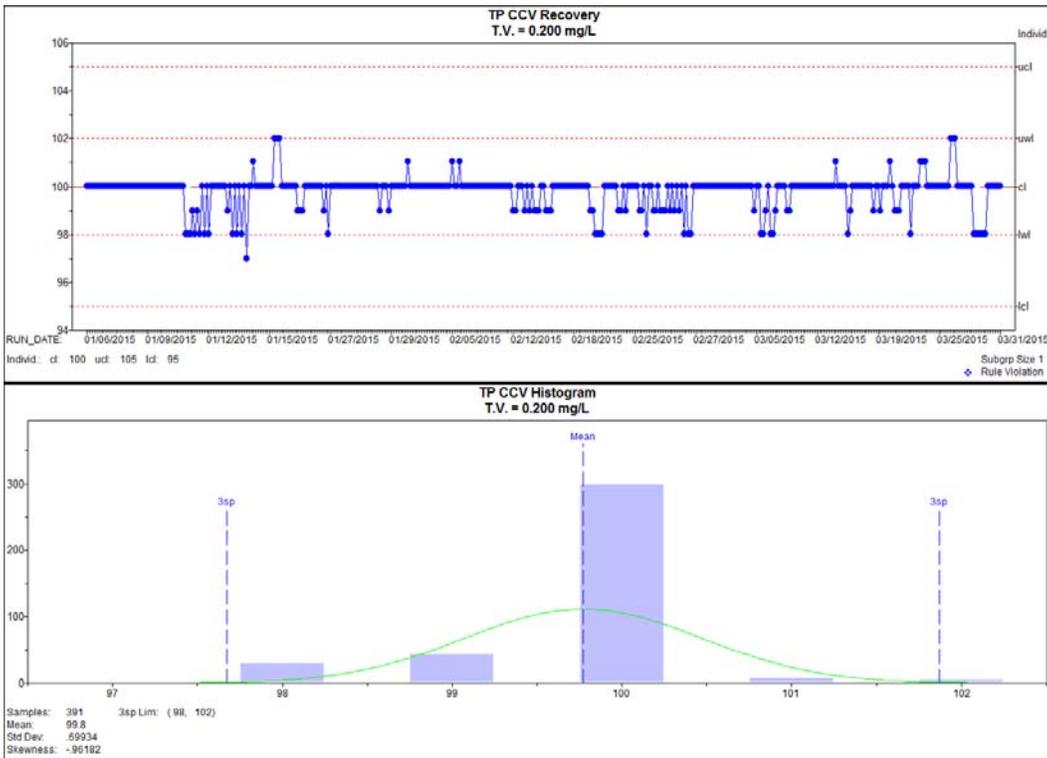


Figure 3. TP QC (Continuing Calibration Verification Sample, 0.200 mg/L) sample recoveries and histogram.

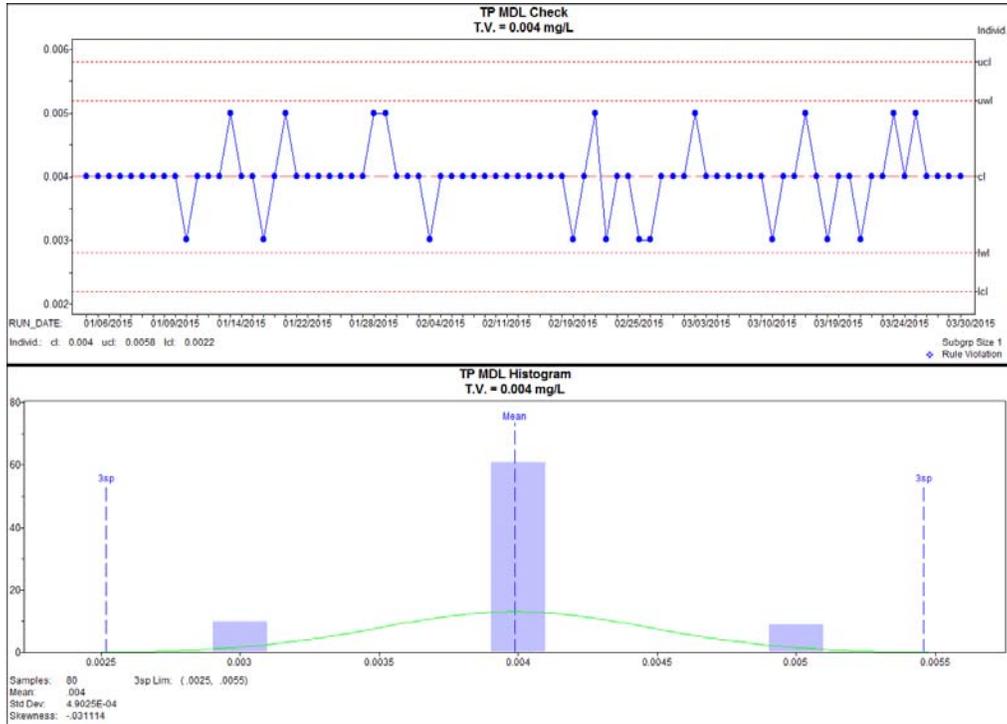


Figure 4. TP QC5 (Method Detection Limit Check, 0.004 mg/L) sample recoveries and histogram.

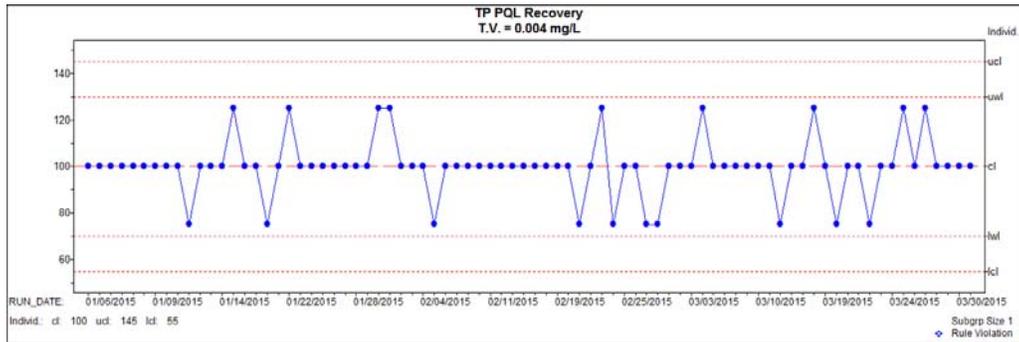


Figure 5. TP PQL (Practical Quantitation Limit) recovery.

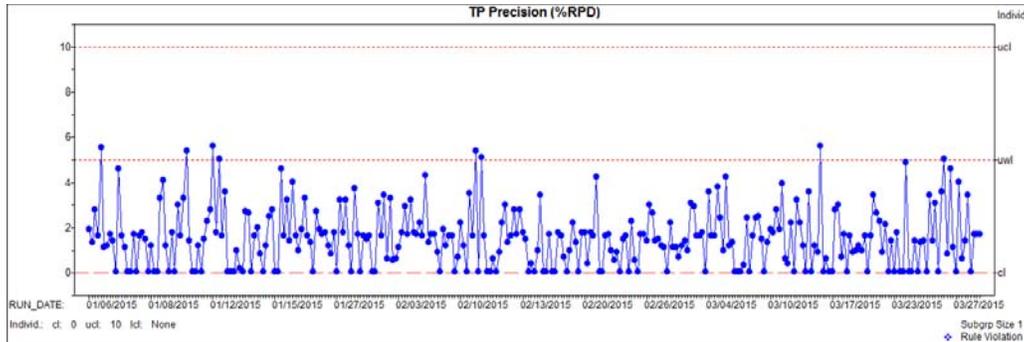


Figure 6. TP precision (%) relative percent different.

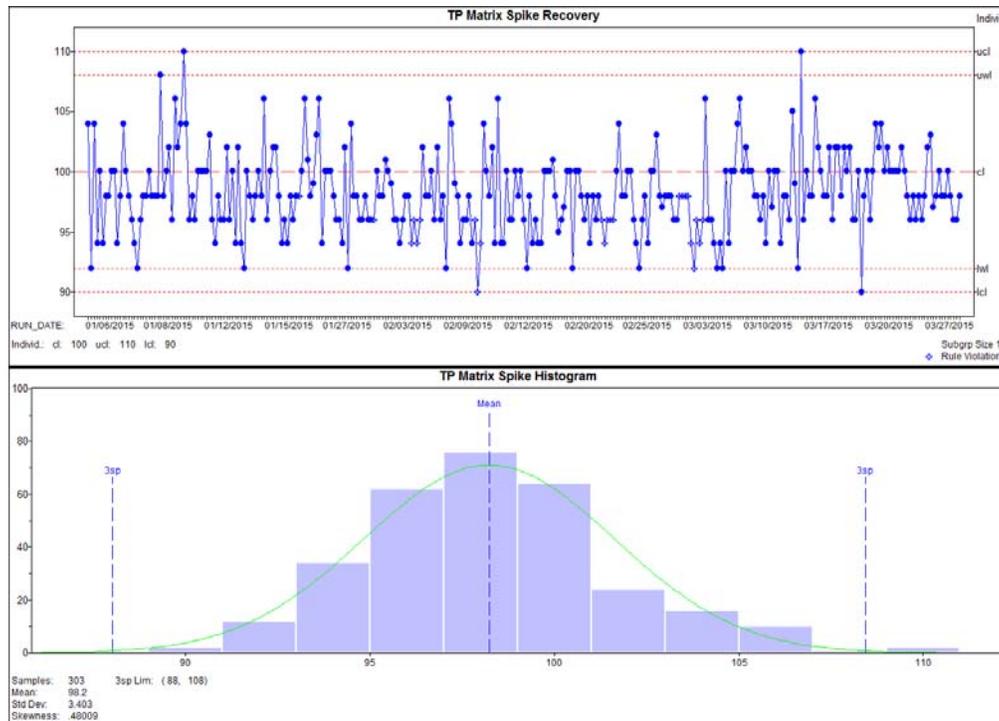


Figure 7. TP spike recovery (%) and histogram.

Notes for Figures 1 through 7:

- T.V. - true value
- ucl - upper control limit
- uwl - upper warning limit
- cl - central line
- lwl - lower warning limit
- lcl - lower control limit
- Min, Max - range of acceptable limits
- Std Dev - standard deviation
- Samples - number of analyzed QC samples
- 3sp Lim - calculated limits for subgroup based on 3 sigma factor
- y-axis label for histogram indicates number of data points

METHOD DETECTION LIMIT AND PRACTICAL QUANTITATION LIMIT

MDL checks are routinely analyzed with each analytical run. From January 1, 2015 to March 31, 2015, 80 results for MDL checks were reported for TP measurements. The calculated MDL from these results was determined to be 0.0012 mg/L, using the procedure described in the Code of Federal Regulations (CFR), Title 40 CFR, Part 136, Appendix B. These results validated the current laboratory MDL value of 0.002 mg/L.

The performance of PQL QC sample is presented in **Figure 5** above. The average recovery for PQL was 98.2 percent. The average relative standard deviation was 12.3 percent, which was less than acceptable criterion of 15 percent. These results validated the current laboratory PQL value of 0.004 mg/L.

The reported values between the MDL (0.002 mg/L) and less than PQL (0.004 mg/L) are assigned the “I” qualifier, indicating that the results are at concentrations that cannot be accurately quantified.

ESTIMATION OF ANALYTICAL MEASUREMENT UNCERTAINTY

The reporting of estimated analytical measurement uncertainty values for all analytes was implemented in July 2012. The definition of uncertainty (of measurement) can be found in the *International Vocabulary of Basic and General Standard Terms in Metrology*: “A parameter associated with the result of a measurement that characterizes the dispersion of the values that could reasonably be attributed to the measurand” (JCGM 1993).

The uncertainty has a probabilistic basis and reflects incomplete knowledge of the quantity. All measurements are subject to uncertainty and a measured value is only complete if it is accompanied by a statement of the associated uncertainty.

The uncertainty has been estimated using the nested hierarchical methodology by Ingersoll (2001) in combination with a mathematical model found in the Eurachem/CITAC (2000) guide on uncertainty. This QC-based nested approach uses the statistical QC data attributed to laboratory measurement activities and does not include uncertainty attributed to field sampling activities. The estimated uncertainty is calculated using the following equation:

$$u(x) = \sqrt{s_0^2 + (s_1^2 x^2)}$$

where:

$u(x)$ is the combined standard uncertainty in the result x .

s_0 is a constant contribution to the overall uncertainty derived from the procedure to determine the MDL.

s_1 is a proportionality constant derived from nested hierarchical methodology by Ingersoll.

Figure 8 is presented to clarify the concept of uncertainty of a measurement process relative to the MDL and PQL.

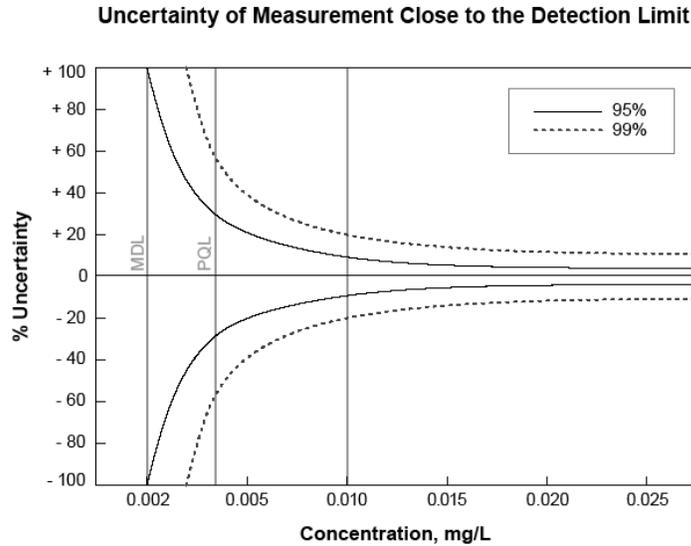


Figure 8. Uncertainty of TP measurement close to the detection limit.

INTER-LABORATORY QUALITY CONTROL ASSESSMENT

SPLIT STUDIES WITH FDEP LABORATORY

To continuously assess comparability of results, the SFWMD routinely sends split samples to other laboratories. **Table 6** contains TP data from the EVPA quarterly splits conducted by the FDEP and the SFWMD laboratories from March 2014 to March 2015.

Effective May 1, 2015, splitting samples from the EVPA project will be discontinued as both the SFWMD lab and FDEP lab are now routinely participating in a performance evaluation program conducted by Environment Canada that provides much more useful statistical information regarding the accuracy and bias of measurements for TP in natural surface waters. The Environment Canada performance evaluation program meets the *Guidelines for the Requirements for the Competence of Providers of Proficiency Testing* (comprising ISO Guide 43-1:1997, as well as relevant elements of ISO/IEC 17025:2005 applicable to characterization, homogeneity and stability testing of proficiency testing materials), and the management system requirements of ISO/IEC 17025:2005, which includes the principles of ISO 9000:2005. For more information on proficiency testing and performance evaluation studies conducted by the SFWMD laboratory, please refer to *Guidance in Implementation of Proficiency Testing and Performance Evaluation Studies*, SFWMD-LAB-G-5610-002, which is available upon request.

Table 6. Comparison of SFWMD and FDEP split TP samples (March 2014–March 2015).

Project Code	Date Collected	Station	SFWMD TP result	FDEP TP result	Relative Percent Difference/Comments
EVPA	3/05/2014	LOX12	0.007±0.002	0.007	0.0
EVPA	3/05/2014	LOX15	0.005±0.002	0.005	0.0
EVPA	3/05/2014	LOX16	0.006±0.002	0.007	15.4
EVPA	3/05/2014	LOX14	0.006±0.002	0.005	18.2
EVPA	6/04/2014	LOX12	0.007±0.002	0.008	13.3
EVPA	6/04/2014	LOX15	0.006±0.002	0.006	0.0
EVPA	6/04/2014	LOX14	0.006±0.002	0.006	0.0
EVPA	6/04/2014	LOX12	0.008±0.002	0.009	11.8
EVPA	9/03/2014	LOX7	0.006±0.002	0.006	0.0
EVPA	9/03/2014	LOX8	0.009±0.002	0.009	0.0
EVPA	9/04/2014	LOX14	0.006±0.002	0.006	0.0
EVPA	9/04/2014	LOX6	0.006±0.002	0.005	18.2
EVPA	12/03/2014	LOX12	0.005±0.002	0.005	0.0
EVPA	12/03/2014	LOX15	0.004±0.002	0.004 (I)	FDEP result < PQL
EVPA	12/03/2014	LOX16	0.005±0.002	0.006	18.2
EVPA	12/03/2014	LOX14	0.005±0.002	0.005	0.0
EVPA	3/03/15	LOX10	0.004±0.002	0.006	40.0
EVPA	3/03/15	LOX9	0.009±0.002	0.009	0.0
EVPA	3/03/15	LOX8	0.007±0.002	0.008	13.3
EVPA	3/03/15	LOX7	0.007±0.002	0.008	13.3

Notes:

SFWMD TP results include analytical uncertainty value

Qualifier code:

I: indicates the reported value is greater than or equal to the MDL but less than PQL.

SFWMD reported MDL = 0.002 mg/L and PQL = 0.004 mg/L

FDEP reported MDL = 0.002 mg/L and PQL = 0.005 mg

National Water Research Institute Environment Canada Ecosystem Inter-laboratory Proficiency Testing Program

Environment Canada provides accredited proficiency program studies for a wide range of inorganic constituents in water. The purpose of the program is to identify sources of measurement uncertainties and variation among analytical results, and to provide information on overall data quality and reliability of analytical measurements of inorganic parameters in natural waters. The results for the SFWMD laboratory from the most recent Proficiency Testing Study 105 are presented in **Table 5** (March 2015). The SFWMD laboratory was rated on performance of TP as “Ideal” (highest). The evaluation includes systematic bias and precision, a laboratory appraisal and a summary of Z-scores (ISO 13528:2005).

The Z-scores, based on the International Organization of Standardization (ISO), Guide 43 can be interpreted as follows:

- $|Z| < 2$ Satisfactory performance
- $2 < |Z| < 3$ Questionable performance
- $|Z| > 3$ Unsatisfactory performance

Table 5. Performance in Proficiency Testing Study 105 for TP, March 2015.

Sample Number	1	2	3	4	5	6	7	8	9	10
Assigned Value, mg/L	0.0442	0.0264	0.1105	0.00579	0.355	0.799	0.00411	0.098	0.002246	0.319
Reported Result, mg/L	0.044	0.263	0.110	0.006	0.358	1.00	0.003	0.099	<0.002	0.319
Z-score	-0.07	-0.11	-0.15	0.16	0.42	2.37	-0.70	0.32	NR	0.00

Notes:

- Assigned Value – this value is the calculated true value of the standard based upon the actual composition of the standard.
- Reported Value – the test result reported to the study provider for a specific analyte.
- NR – Not Ranked

REFERENCES

- Eurachem/CITAC. 2000. *Quantifying Uncertainty in Analytical Measurement, Second Edition*. ISBN 0-948926-15-5, Eurachem/CITAC, Guide CG4.
- Ingersoll, W.S. 2001. Environmental Analytical Measurement Uncertainty Estimation. Nested Hierarchical Approach. Defense Technical Information Center #ADA396946, Fort Belvoir, VA.
- ISO. 1997. *ISO/IEC Guide 43-1: 1997, Proficiency Testing by Interlaboratory Comparisons -- Part 1: Development and Operation of Proficiency Testing Schemes*. International Organization for Standardization. Available at http://www.iso.org/iso/iso_catalogue/catalogue_ics/catalogue_detail_ics.htm?csnumber=27216.
- ISO. 2009. *ISO 9000/2005, Quality Management Systems -- Fundamentals and Vocabulary*. International Organization for Standardization. Available at http://www.iso.org/iso/home/store/catalogue_tc/catalogue_detail.htm?csnumber=42180.
- ISO. 2010. *ISO/IEC 17025:2005, General Requirements for the Competence of Testing and Calibration Laboratories*. International Organization for Standardization. Available at http://www.iso.org/iso/home/store/catalogue_tc/catalogue_detail.htm?csnumber=39883.
- JCGM. 1993. *International Vocabulary of Basic and General Standard Terms in Metrology*. Joint Committee on Guides for Metrology, Geneva, Switzerland (ISBN 92-67-10175-1).
- SFWMD. 2010. *Guidance in Implementation of Proficiency Testing and Performance Evaluation Studies*. SFWMD-LAB-G-5610-002, South Florida Water Management District, West Palm Beach, FL. April 14, 2010.

SFWMD. 2015a. Chemistry Laboratory Quality Manual, SFWMD-LAB-QM-2015-01. South Florida Water Management District, West Palm Beach, FL.

SFWMD. 2015b. Field Sampling Quality Manual, SFWMD-FIELD-QM-001-08.2. South Florida Water Management District, West Palm Beach, FL.

GLOSSARY

Accuracy: The degree of agreement between an observed value and an accepted reference value. Accuracy includes a combination of random error (precision) and systematic error (bias) components that are due to sampling and analytical operations.

Equipment Blank (EB): Field QC sample prepared using sampling equipment that has been brought to the site or processing area precleaned and is collected before the equipment has been used. The results of these blanks are used to monitor the on-site sampling environment, sampling equipment decontamination, sample container cleaning, the suitability of sample preservatives and analyte-free water, sample transport and storage conditions, and laboratory process.

Field Blank (FB): FBs are collected by pouring analyte-free water directly into the sample container, preserved, and kept open for the same approximate time and interval as required for collection and/or processing of the routine sample. The results of this blank are used to monitor the on-site sampling environment, sample container cleaning, the suitability of sample preservatives and analyte-free water, sample transport and storage conditions, and laboratory process.

Field Cleaned Equipment Blank (FCEB): Field QC sample prepared using sampling equipment that has been cleaned in the field or at the processing area. The results of this blank are used to monitor the on-site sampling environment, sampling equipment field decontamination, sample container cleaning, the suitability of sample preservatives and analyte-free water, sample transport and storage conditions, and laboratory process.

Measurand: Particular quantity subject to measurement.

Method Detection Limit (MDL): The smallest concentration of an analyte of interest that can be measured and reported with 99 percent confidence that the concentration is greater than zero. The MDLs are determined from the analysis of a sample in a given matrix, using accepted sampling and analytical preparation procedures, containing the analyte at a specified level. The MDL is determined by the protocol defined in the Code of Federal Regulations (CFR) section 40 CFR, Part 136, Appendix B, as established by the United States Environmental Protection Agency.

Practical Quantitation Limit (PQL): The smallest concentration of an analyte of interest that can be quantitatively reported with a specific degree of confidence. The PQL is verified for each matrix, technology and analyte. The validity of the PQL is verified by analysis of quality control sample containing the analyte of concern.

Precision: The agreement or closeness between two or more results and is an indication that the measurement system is operating consistently and is a quantifiable indication of variations introduced by the analytical systems over a given time and field sampling period.

Relative Percent Difference (RPD): A measure of precision, used when comparing two values. It is calculated as $\%RPD = [Value1 - Value2] / Mean * 100$.

Relative Standard Deviation (RSD): A measurement of precision, used when comparing more than two results. It is calculated as $\%RSD = [Standard Deviation / Mean] * 100$.

Replicate Sample (RS): A RS is collected by repeating (simultaneously or in rapid succession) the entire sample acquisition technique that was used to obtain the routine sample. A single RS set (e.g., one sample and two RS) is collected per quarter, per project, at the same station, for the longest parameter list. RS data are compared to routine sample data to evaluate sampling precision.

Split Sample (SS): A second sample collected from the same sample obtained from the same sampling device. Results for SS are compared with routine sample results; agreement between these two results is mostly an indication of laboratory precision.

Uncertainty: The range of values within which the true value is estimated to lie. It is a best estimate of possible inaccuracy due to both random and systematic error.

Z-Score: A measure of the deviation of the result (X_i) from the assigned value (X) for that determinant (calculated as $z = (X_i - X) / \sigma$, where σ is a standard deviation) (Eurachem/CITAC 2000).

APPENDIX B

TP results for projects and their associated stations specified in the Introduction from January 1, 2015, to March 31, 2015. Among 122 reported results, 11 were qualified with a code "I".

Project	Date Collected	Station	TP Result (mg/L)	Uncertainty (mg/L)	Qualifier Code
PIN	1/5/2015	S12A	0.014	+/- 0.002	
PIN	1/5/2015	S333	0.010	+/- 0.002	
PIN	1/5/2015	S356-334	0.009	+/- 0.002	
PIE	1/5/2015	S332DX	0.005	+/- 0.002	
EVPA	1/6/2015	LOX3	0.009	+/- 0.002	
EVPA	1/6/2015	LOX5	0.010	+/- 0.002	
EVPA	1/6/2015	LOX10	0.007	+/- 0.002	
EVPA	1/6/2015	LOX9	0.009	+/- 0.002	
EVPA	1/6/2015	LOX8	0.009	+/- 0.002	
EVPA	1/6/2015	LOX7	0.009	+/- 0.002	
EVPA	1/6/2015	LOX4	0.009	+/- 0.002	
PIN	1/6/2015	S355A	0.017	+/- 0.002	
PIN	1/6/2015	S355B	0.018	+/- 0.002	
PIE	1/6/2015	S18C	0.002	+/- 0.002	I
EVPA	1/8/2015	LOX12	0.008	+/- 0.002	
EVPA	1/8/2015	LOX15	0.007	+/- 0.002	
EVPA	1/8/2015	LOX16	0.008	+/- 0.002	
EVPA	1/8/2015	LOX14	0.007	+/- 0.002	
EVPA	1/8/2015	LOX13	0.007	+/- 0.002	
EVPA	1/8/2015	LOX11	0.009	+/- 0.002	
EVPA	1/8/2015	LOX6	0.006	+/- 0.002	
PIN	1/12/2015	S12A	0.010	+/- 0.002	
PIN	1/12/2015	S12D	0.010	+/- 0.002	
PIN	1/12/2015	S356-334	0.008	+/- 0.002	
PIN	1/12/2015	S333	0.010	+/- 0.002	
PIE	1/12/2015	S332DX	0.006	+/- 0.002	
PIE	1/13/2015	S18C	0.003	+/- 0.002	I
PIN	1/20/2015	S12A	0.016	+/- 0.002	
PIN	1/20/2015	S12D	0.009	+/- 0.002	
PIN	1/20/2015	S333	0.011	+/- 0.002	
PIN	1/20/2015	S356-334	0.009	+/- 0.002	
PIE	1/20/2015	S332DX	0.005	+/- 0.002	
PIE	1/20/2015	S18C	0.003	+/- 0.002	I
PIN	1/22/2015	S355A	0.012	+/- 0.002	
PIN	1/22/2015	S355B	0.012	+/- 0.002	
PIE	1/26/2015	S332DX	0.005	+/- 0.002	
PIN	1/26/2015	S12A	0.011	+/- 0.002	
PIN	1/26/2015	S12D	0.007	+/- 0.002	
PIN	1/26/2015	S356-334	0.007	+/- 0.002	
PIE	1/27/2015	S18C	0.003	+/- 0.002	I
PIN	2/2/2015	S12A	0.008	+/- 0.002	
PIN	2/2/2015	S12D	0.008	+/- 0.002	
PIN	2/2/2015	S356-334	0.009	+/- 0.002	
PIE	2/2/2015	S332DX	0.005	+/- 0.002	
EVPA	2/3/2015	LOX4	0.006	+/- 0.002	
EVPA	2/3/2015	LOX7	0.006	+/- 0.002	
EVPA	2/3/2015	LOX8	0.009	+/- 0.002	
EVPA	2/3/2015	LOX9	0.006	+/- 0.002	
EVPA	2/3/2015	LOX10	0.004	+/- 0.002	
EVPA	2/3/2015	LOX5	0.009	+/- 0.002	
EVPA	2/3/2015	LOX3	0.010	+/- 0.002	

Project	Date Collected	Station	TP Result (mg/L)	Uncertainty (mg/L)	Qualifier Code
PIE	2/3/2015	S18C	0.002	+/- 0.002	I
PIN	2/3/2015	S355A	0.009	+/- 0.002	
PIN	2/3/2015	S355B	0.012	+/- 0.002	
EVPA	2/4/2015	LOX12	0.005	+/- 0.002	
EVPA	2/4/2015	LOX15	0.003	+/- 0.002	I
EVPA	2/4/2015	LOX16	0.005	+/- 0.002	
EVPA	2/4/2015	LOX14	0.005	+/- 0.002	
EVPA	2/4/2015	LOX13	0.004	+/- 0.002	
EVPA	2/4/2015	LOX11	0.005	+/- 0.002	
EVPA	2/4/2015	LOX6	0.004	+/- 0.002	
PIN	2/9/2015	S12A	0.009	+/- 0.002	
PIN	2/9/2015	S12D	0.009	+/- 0.002	
PIN	2/9/2015	S356-334	0.008	+/- 0.002	
PIE	2/9/2015	S332DX	0.007	+/- 0.002	
PIE	2/10/2015	S18C	0.002	+/- 0.002	I
PIN	2/16/2015	S12A	0.008	+/- 0.002	
PIN	2/16/2015	S12D	0.008	+/- 0.002	
PIE	2/16/2015	S332DX	0.006	+/- 0.002	
PIN	2/16/2015	S356-334	0.007	+/- 0.002	
PIE	2/17/2015	S18C	0.003	+/- 0.002	I
PIN	2/18/2015	S355A	0.010	+/- 0.002	
PIN	2/18/2015	S355B	0.010	+/- 0.002	
PIN	2/23/2015	S12A	0.007	+/- 0.002	
PIN	2/23/2015	S12D	0.007	+/- 0.002	
PIN	2/23/2015	S356-334	0.008	+/- 0.002	
PIE	2/23/2015	S332DX	0.005	+/- 0.002	
PIE	2/24/2015	S18C	0.003	+/- 0.002	I
PIN	3/2/2015	S12A	0.009	+/- 0.002	
PIN	3/2/2015	S12D	0.011	+/- 0.002	
PIE	3/2/2015	S332DX	0.005	+/- 0.002	
PIN	3/2/2015	S356-334	0.007	+/- 0.002	
EVPA	3/3/2015	LOX3	0.011	+/- 0.002	
EVPA	3/3/2015	LOX5	0.010	+/- 0.002	
EVPA	3/3/2015	LOX10	0.004	+/- 0.002	
EVPA	3/3/2015	LOX9	0.009	+/- 0.002	
EVPA	3/3/2015	LOX8	0.007	+/- 0.002	
EVPA	3/3/2015	LOX7	0.007	+/- 0.002	
EVPA	3/3/2015	LOX4	0.009	+/- 0.002	
PIN	3/3/2015	S355A	0.010	+/- 0.002	
PIN	3/3/2015	S355B	0.012	+/- 0.002	
PIE	3/3/2015	S18C	0.004	+/- 0.002	
EVPA	3/4/2015	LOX12	0.007	+/- 0.002	
EVPA	3/4/2015	LOX15	0.005	+/- 0.002	
EVPA	3/4/2015	LOX16	0.008	+/- 0.002	
EVPA	3/4/2015	LOX14	0.006	+/- 0.002	
EVPA	3/4/2015	LOX13	0.006	+/- 0.002	
EVPA	3/4/2015	LOX11	0.006	+/- 0.002	
EVPA	3/4/2015	LOX6	0.006	+/- 0.002	
PIN	3/9/2015	S12A	0.012	+/- 0.002	
PIN	3/9/2015	S12D	0.011	+/- 0.002	
PIN	3/9/2015	S333	0.011	+/- 0.002	
PIN	3/9/2015	S356-334	0.009	+/- 0.002	
PIE	3/9/2015	S332DX	0.008	+/- 0.002	
PIE	3/10/2015	S18C	0.003	+/- 0.002	I
PIN	3/16/2015	S12A	0.015	+/- 0.002	
PIN	3/16/2015	S333	0.011	+/- 0.002	
PIN	3/16/2015	S356-334	0.012	+/- 0.002	
PIE	3/16/2015	S332DX	0.008	+/- 0.002	
PIN	3/17/2015	S355A	0.012	+/- 0.002	

Project	Date Collected	Station	TP Result (mg/L)	Uncertainty (mg/L)	Qualifier Code
PIE	3/17/2015	S18C	0.004	+/- 0.002	
PIN	3/17/2015	S355B	0.012	+/- 0.002	
PIN	3/23/2015	S12A	0.017	+/- 0.002	
PIN	3/23/2015	S333	0.010	+/- 0.002	
PIN	3/23/2015	S356-334	0.012	+/- 0.002	
PIE	3/23/2015	S332DX	0.010	+/- 0.002	
PIE	3/24/2015	S18C	0.003	+/- 0.002	I
PIN	3/30/2015	S12A	0.012	+/- 0.002	
PIE	3/30/2015	S332DX	0.009	+/- 0.002	
PIN	3/30/2015	S333	0.012	+/- 0.002	
PIN	3/30/2015	S356-334	0.010	+/- 0.002	
PIE	3/31/2015	S18C	0.007	+/- 0.002	

Notes:

Qualifier code:

I indicates the reported value is greater than or equal to the MDL but less than PQL.